

Explainable Image Quality Analysis of Chest X-Rays






Caner Ozer, Ilkay Oksuz

Motivation


- ❖ Accelerating image acquisition procedure by proposing an automated foreign object classification system on Chest X-Rays
- ❖ Ensuring that the whole system is interpretable for a potential clinical translation
- ❖ Verifying the interpretation method is accurate and using the ground truth bounding box annotations for only evaluation purposes

Methodology

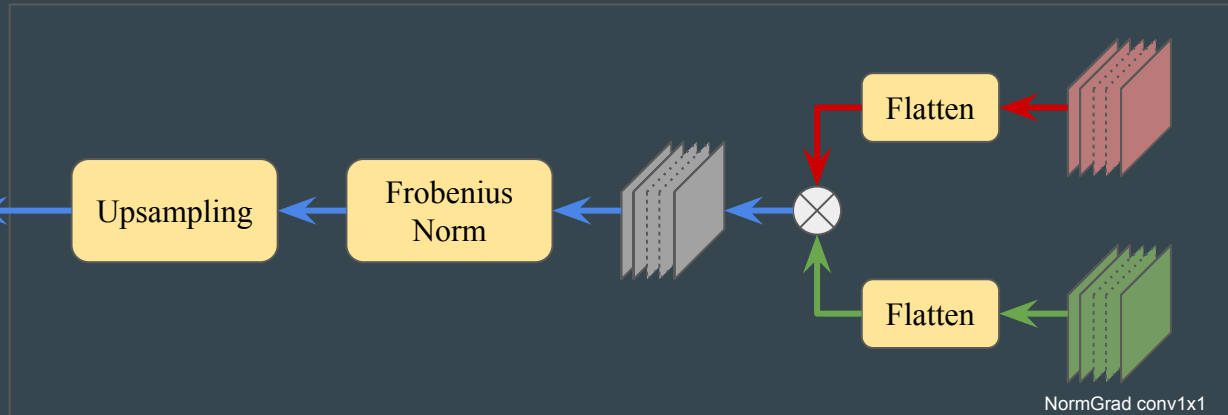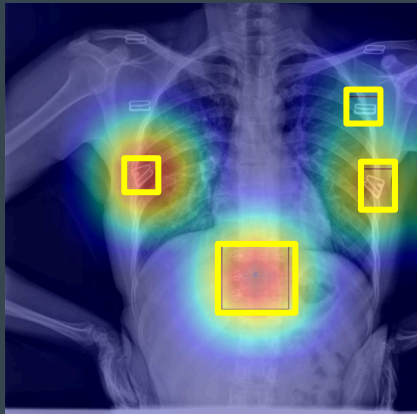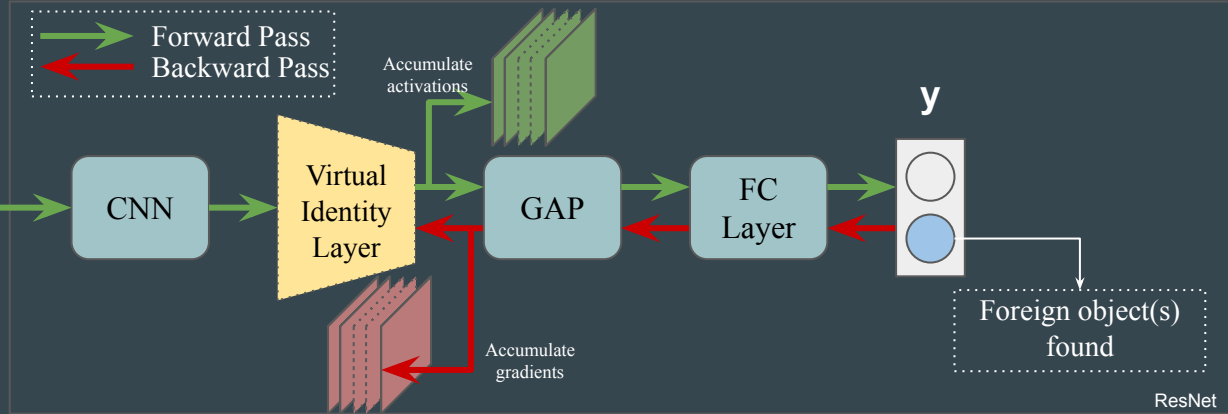


Comparison with Baseline Models

Method	Object-CXR Val	Object-CXR Test
Input x Gradient (Shrikumar et al., ICML'17)	0.246	0.24
Guided Backpropagation (Springenberg et al., ICLR'15)	0.208	0.188
Guided Grad-CAM (Selvaraju et. al., IJCV'20)	0.348	0.334
Grad-CAM (Selvaraju et. al., IJCV'20)	0.684	0.656
NormGrad (conv4.2, conv3x3) (Rebuffi et. al., CVPR'20)	0.874	0.862
NormGrad (Combined, conv3x3) (Rebuffi et. al., CVPR'20)	0.88	0.85

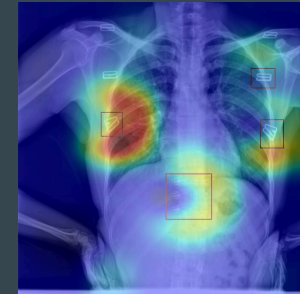

Grad-CAM

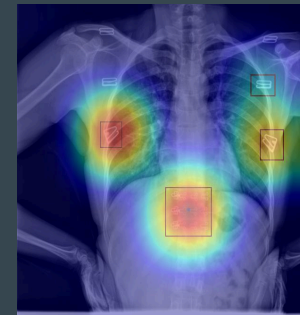

NormGrad